


# ANSI A326.3 Report

Regan Scientific Instruments


03/12/2024, 11:53AM

Method: DCOF  
Product: 001  
Specimen: 001  
Result: 0.57  
Distance: 08 in.  
Temp/Hum: 70 F, 35%  
Type: Lab/Dry  
Condition: Clean


1. Avg = 0.55, Min = 0.49, Max = 0.60

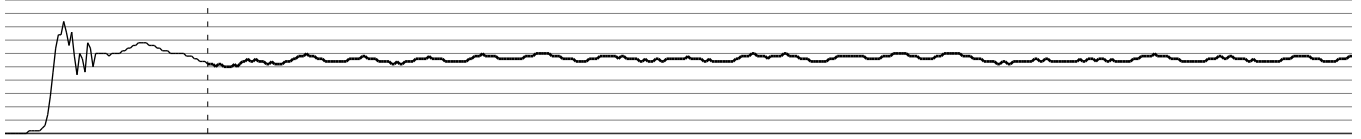


2. Avg = 0.58, Min = 0.52, Max = 0.64

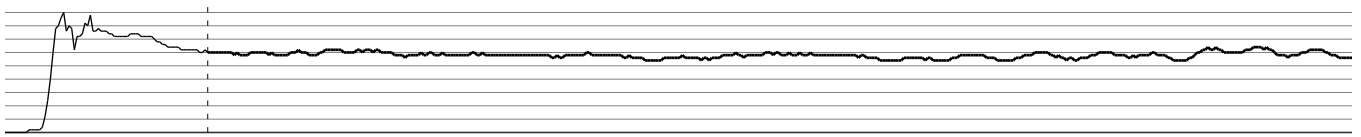

3. Avg = 0.58, Min = 0.52, Max = 0.62

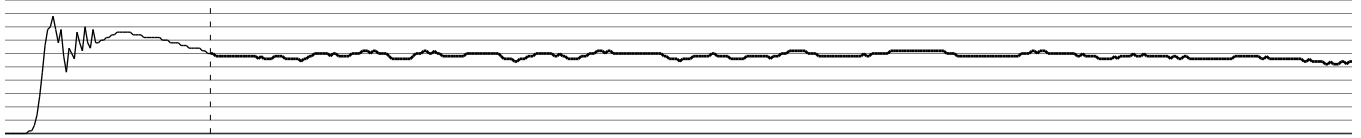

4. Avg = 0.56, Min = 0.50, Max = 0.59

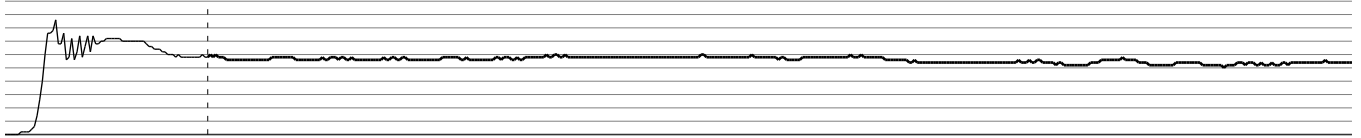

Device: BOT-3000E (v3.00.08)  
Serial No: 00569  
Calibration: 04/14/2023  
Verification: 03/12/2024, 8:13AM PASS  
Meter: 28.4 hrs

Sensor: 00887  
Type: Rubber  
Manuf. date: 08/19/2021  
Ref. offset: ----


# ANSI A326.3 Report

Regan Scientific Instruments


03/12/2024, 11:55AM

Method: DCOF  
Product: 001  
Specimen: 002  
Result: 0.54  
Distance: 08 in.  
Temp/Hum: 70 F, 35%  
Type: Lab/Dry  
Condition: Clean


1. Avg = 0.53, Min = 0.49, Max = 0.63

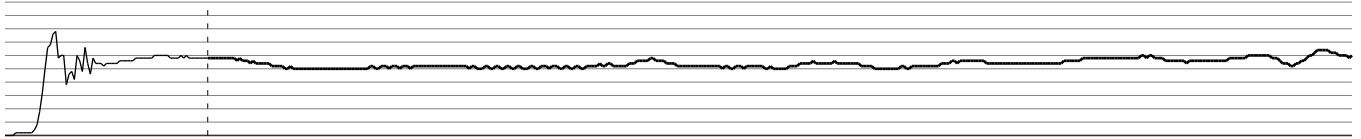


2. Avg = 0.57, Min = 0.51, Max = 0.67

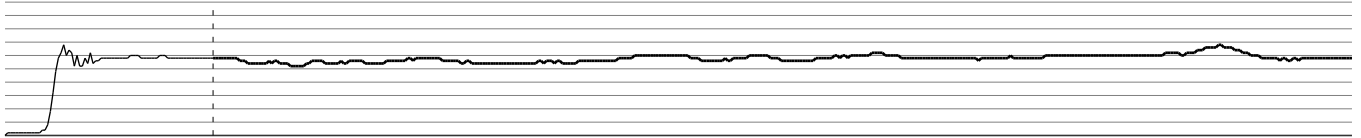

3. Avg = 0.54, Min = 0.48, Max = 0.60

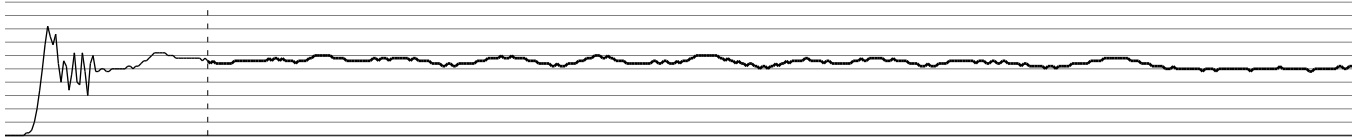

4. Avg = 0.53, Min = 0.48, Max = 0.59

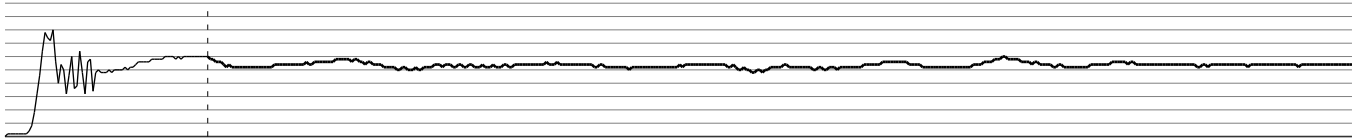

Device: BOT-3000E (v3.00.08)  
Serial No: 00569  
Calibration: 04/14/2023  
Verification: 03/12/2024, 8:13AM PASS  
Meter: 28.4 hrs

Sensor: 00887  
Type: Rubber  
Manuf. date: 08/19/2021  
Ref. offset: ----


# ANSI A326.3 Report

Regan Scientific Instruments


03/12/2024, 11:56AM

Method: DCOF  
Product: 001  
Specimen: 003  
Result: 0.50  
Distance: 08 in.  
Temp/Hum: 70 F, 35%  
Type: Lab/Dry  
Condition: Clean


1. Avg = 0.51, Min = 0.47, Max = 0.53

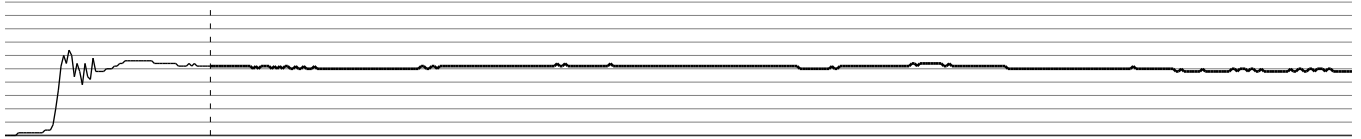


2. Avg = 0.51, Min = 0.47, Max = 0.56

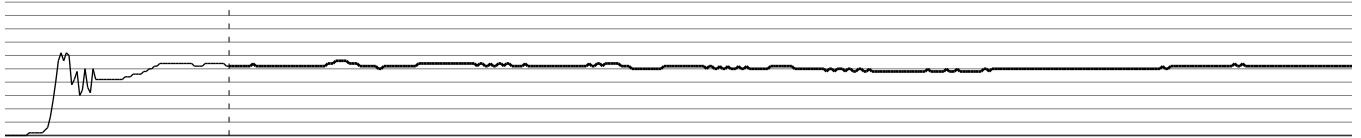

3. Avg = 0.48, Min = 0.45, Max = 0.51

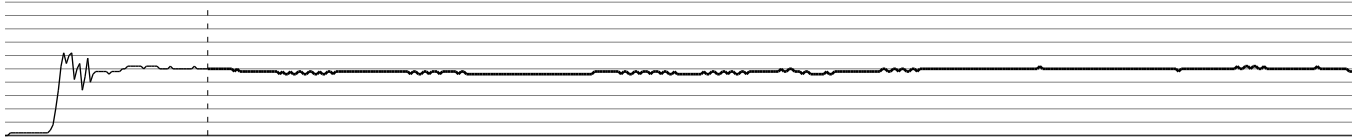

4. Avg = 0.50, Min = 0.47, Max = 0.53

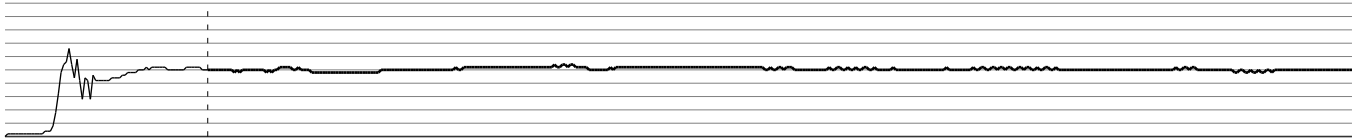

Device: BOT-3000E (v3.00.08)  
Serial No: 00569  
Calibration: 04/14/2023  
Verification: 03/12/2024, 8:13AM PASS  
Meter: 28.4 hrs

Sensor: 00887  
Type: Rubber  
Manuf. date: 08/19/2021  
Ref. offset: ----